


ECM Rackmount Panel Kit, P/N 12-01, Installation Instructions




1. Remove the two screws on the back panel of the 5200 series instrument.





2. Slide the back panel and the main board out of the instrument. Do not separate the back panel from the main board.




3. Remove the two screws on the front panel and separate the aluminum base, the top cover, the front display, and the bezel.

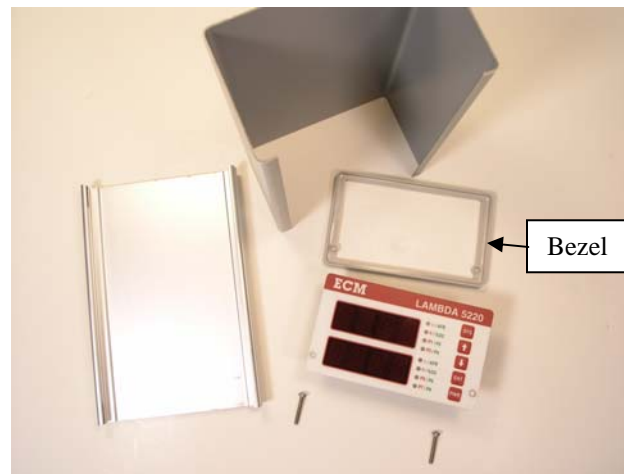


4. Sandwich the rackmount panel, WITHOUT THE FRONT BEZEL, between the front display and the aluminum base. Reinstall the two front screws. Do not overtighten the front screws or you will damage the front panel.

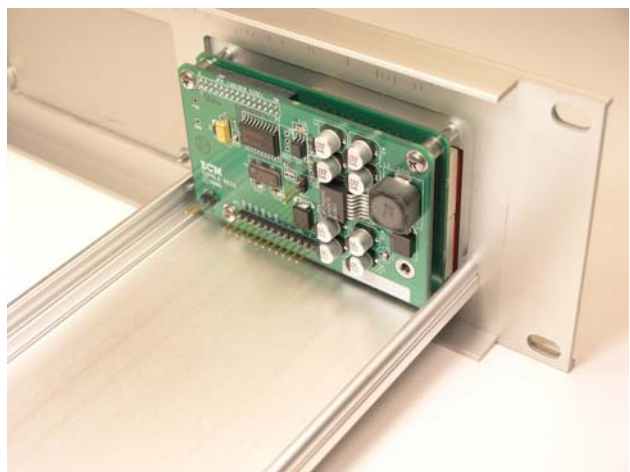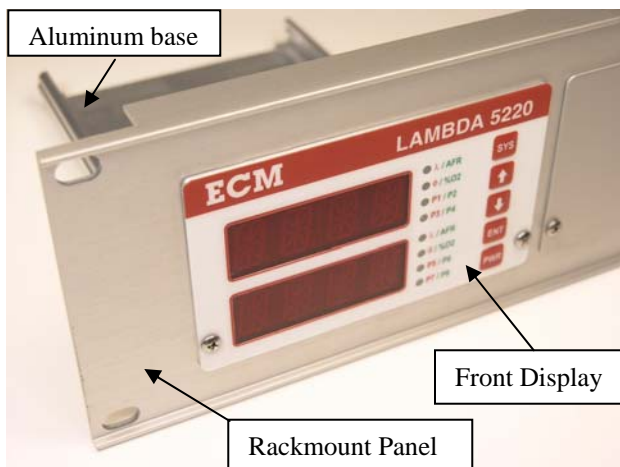

5. Install the top cover onto the aluminum base and slide it up to the front. Make sure the top cover fits into the correct grooves in the aluminum base.

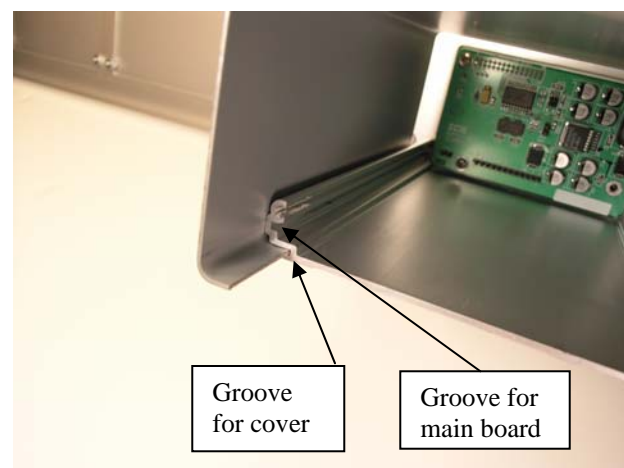

6. To store the front bezel, put it on top of the main board and slide the back panel and the main board into the instrument. Make sure that the main board fits into the grooves in the aluminum base. Just before the main board is fully inserted, you will start to feel the pins of the front display going into the connectors on the main board. Do not force it and if it feels unusual, slide the main board out to inspect the pins in the front display. If you bend them, return the instrument to ECM for repair.

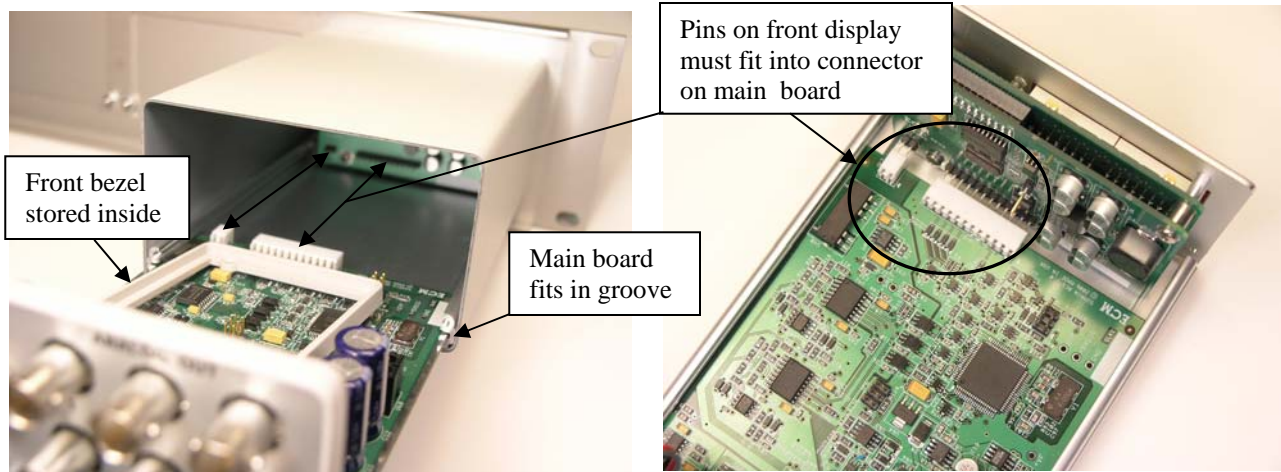

7. Reinstall the two back screws.



ECM_RackmountKit12-01.doc
© ECM, 2007
Los Altos, CA USA
408-734-3433
www.ecm-co.com